




# SwiftNINJA<sup>®</sup>

Steerable Coronary  
Microcatheter

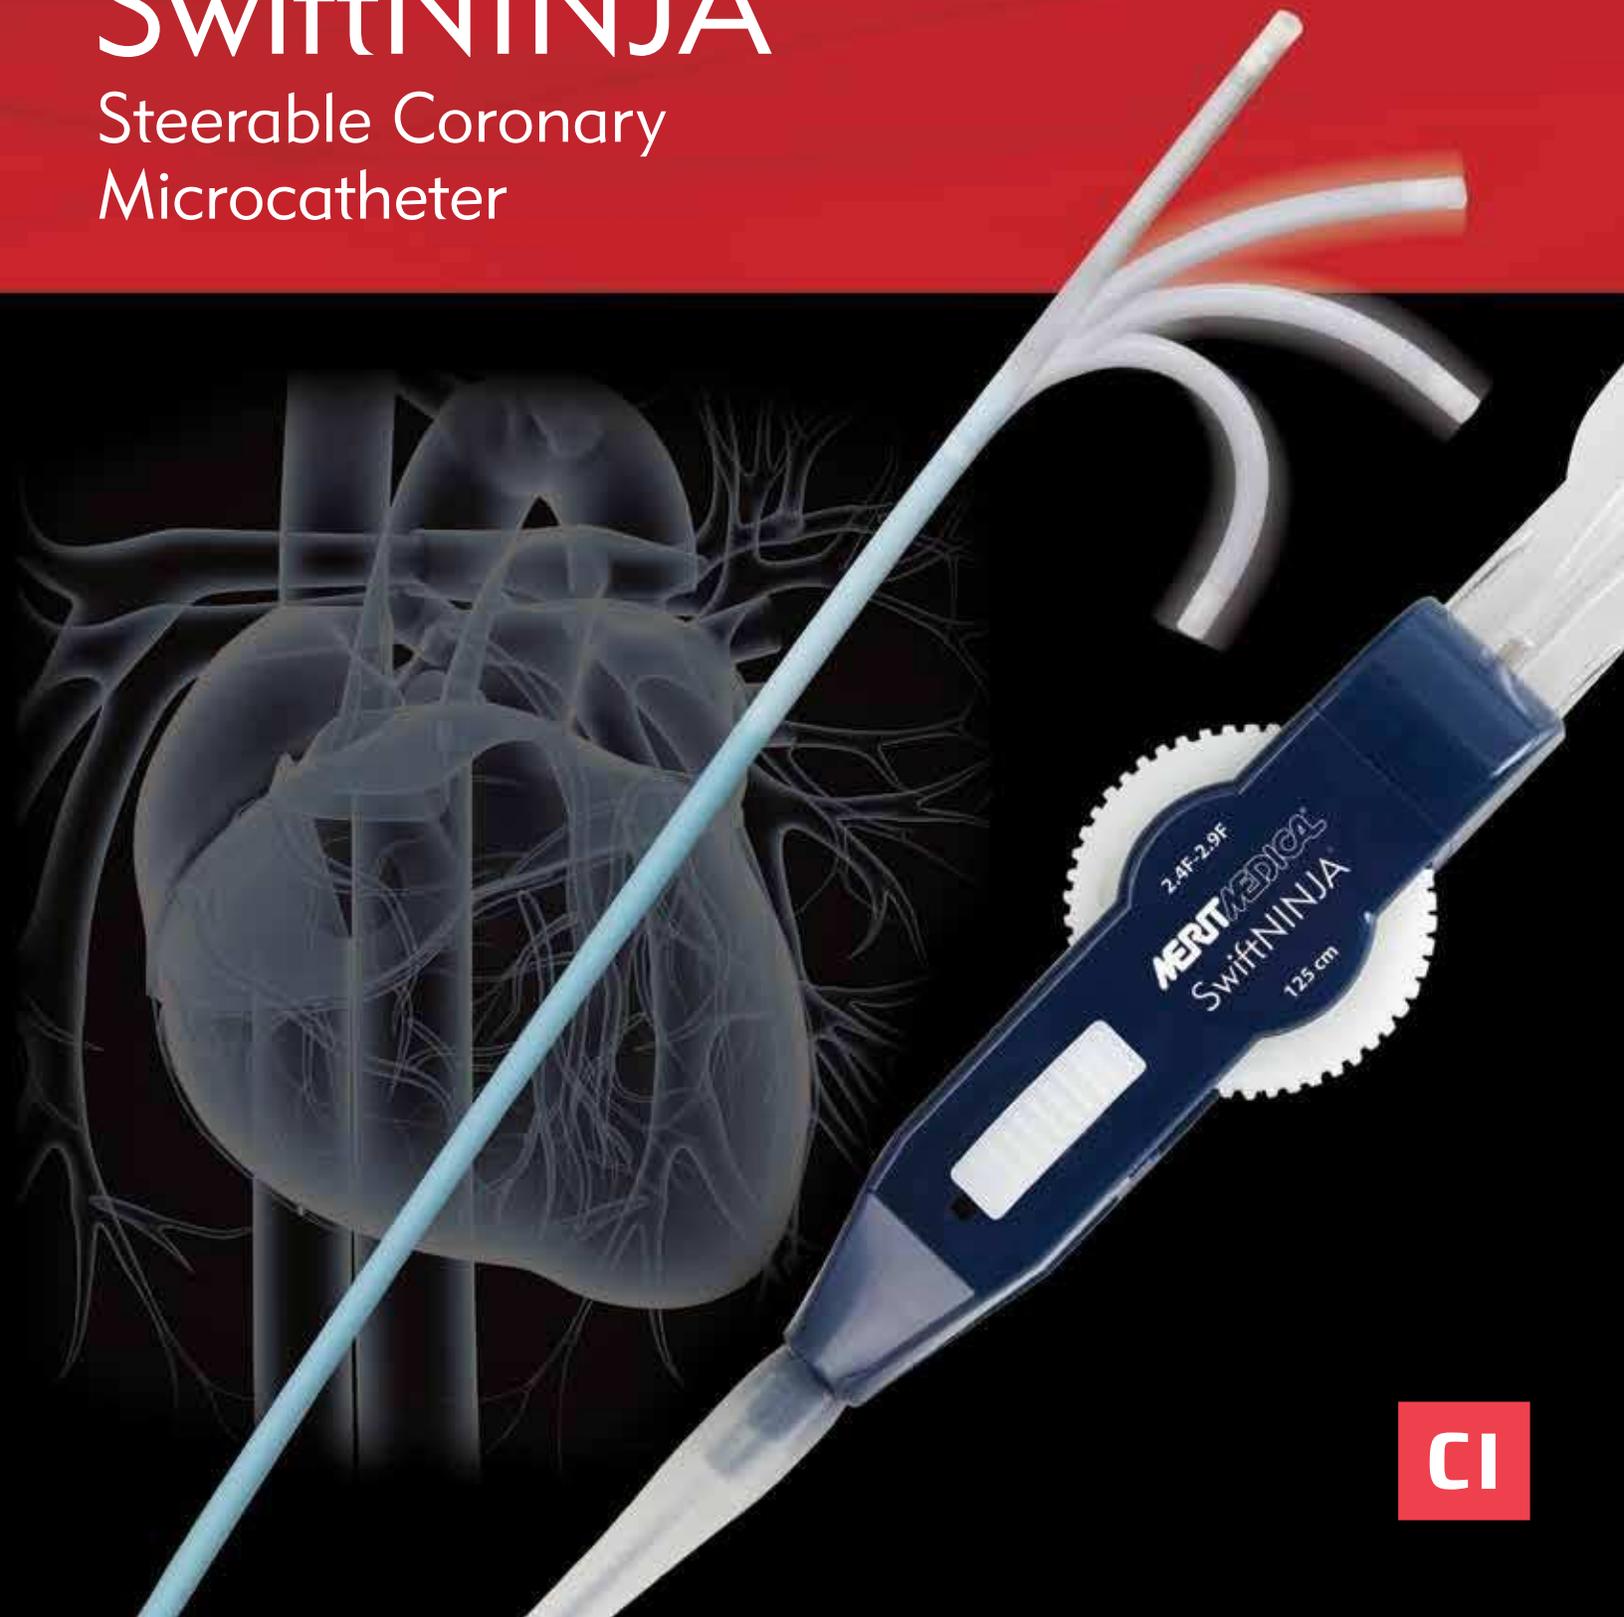


# SwiftNINJA<sup>®</sup>

Steerable Coronary Microcatheter


## SwiftNINJA<sup>®</sup>

The most advanced and only 180° articulating coronary and peripheral vascular microcatheter on the market today. Speed, control, support and navigation at your fingertips.

Hydrophilic coating  
on distal 80 cm

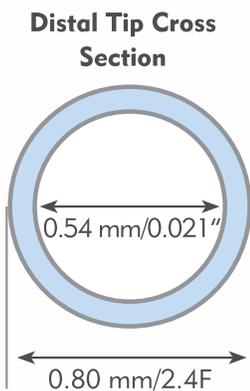

## Close-up of Steerable Tip

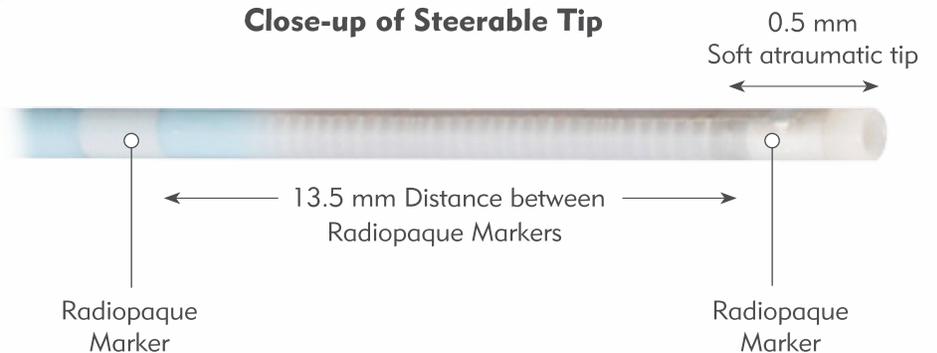

## Fluoroscopic Visualization


Two radiopaque marker bands  
for enhanced navigation and  
tip placement

## INNOVATIVE DESIGN

Innovative microtechnology designed to articulate in opposing directions to navigate the most challenging vascular anatomy.


### Steering Dial Mechanism

Allows opposing 180° articulation from neutral

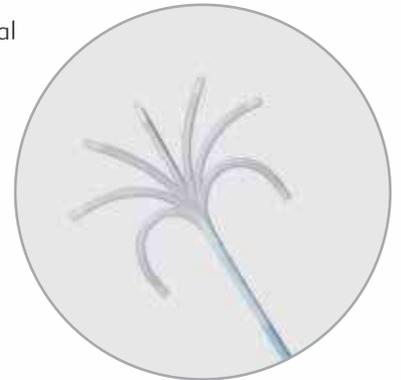

### Steering Lock

Once shaped, the tip can be locked in position

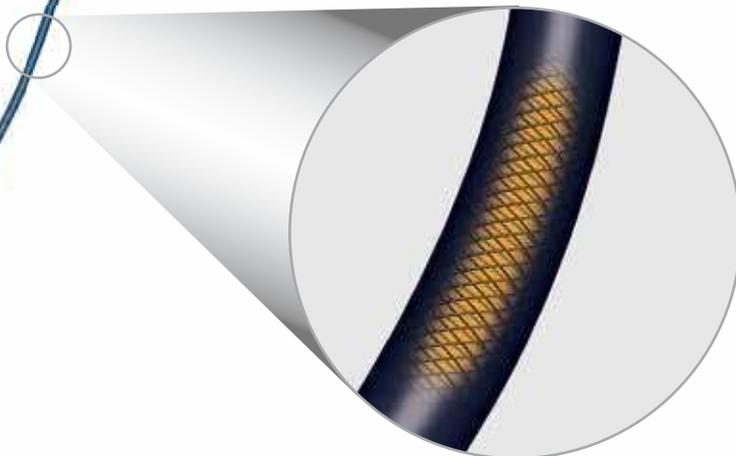

### Tungsten-braided Shaft

Braided shaft enhances shaft support and provides pushability

# SwiftNINJA®

## Steerable Coronary Microcatheter



### Catheter Specifications

Part Number	Inner Diameter	Outer Diameter Proximal Portion	Outer Diameter Distal Portion	Usable Length	Hydrophilic Coating Length	Max Guide wire	Maximum Injection Pressure	Distance From Tip To 1 <sup>st</sup> Markerband	Distance Between 1 <sup>st</sup> And 2 <sup>nd</sup> Markerbands	Cath Vol.
SNCM125	0.021" (0.54 mm)	2.9F (0.97 mm)	2.4F (0.80 mm)	125 cm	80 cm	≤ 0.018" (0.46 mm)	6,900 kPa (1,000 psi)	0.5 mm	13.5 mm	0.49 mL

### Catheter Preparation for Use

To activate the hydrophilic coating: Flush the catheter with heparinized saline via the standard luer BEFORE removal from the protective catheter sleeve.

To Unlock Steering Dial (white wheel): Hold the lower housing body and gently pull the steering dial toward the luer connector until a clicking sound is heard.



Prior to attempting catheter tip movement or deflection, you must engage the steering dial

### Ordering Information:

Part Number	Description
SNCM125	SwiftNINJA® Steerable Coronary Microcatheter 2.9F-2.4F 125 cm



Before using, refer to Instructions for Use for indications, contraindications, warnings, precautions and directions for use.



Understand. Innovate. Deliver.™

Merit Medical Systems, Inc.  
1600 West Merit Parkway  
South Jordan, Utah 84095  
1.801.208.4300  
1.800.35.MERIT

merit.com

Merit Medical Europe, Middle East, & Africa (EMEA)  
Amerikalaan 42, 6199 AE Maastricht-Airport  
The Netherlands  
+31 43 358 82 22

Merit Medical Ireland Ltd.  
Parkmore Business Park West  
Galway, Ireland  
+353 (0) 91 703 733

Australia  
+61 (0) 3 8373 4943

Austria  
0800 295 374

Belgium  
0800 72 906 (Dutch)  
0800 73 172 (Français)

Brazil  
+55 11 4561 - 0062

Canada  
1.800.364.4370

China  
+86-10 8561 0788

Denmark  
80 88 00 24

Finland  
0800 770 586

France  
0800 91 60 30

Germany  
0800 182 0871

Hong Kong  
+852-2207 6888

India  
+91-80-41223376

Ireland (Republic)  
1800 553 163

Italy  
800 897 005

Korea  
+8210 2205 0707

Luxembourg  
8002 25 22

Netherlands  
0800 022 81 84

Norway  
800 11629

Portugal  
308 801 034

Russia  
+7 495 221 89 02

Spain  
+34 911238406

Sweden  
020 792 445

Switzerland  
(Deutsch)  
+41 22 518 02 30

(Français)  
+41 22 518 02 52

(Italiano)  
+41 22 518 00 35

UK  
0800 973 115